



Reduce Your Disinfection Operating Costs

Hi there,

Thank you for your interest in the ASTRA TEE Automated Probe Reprocessor. This report compares the 5-year cost of ownership based on the 70 probes you estimated that you reprocess per week.


ASTRA is designed to standardize your disinfection processes, improve staff workflow, and comply with evidence-based guidelines, while helping you confidently achieve patient and staff safety at your facility.

Contact your CIVCO Account Representative at 800.445.6741 to learn more.

Sincerely,

CIVCO Medical Solutions

You Could Save \$180,299.11
Over 5 Years With ASTRA TEE

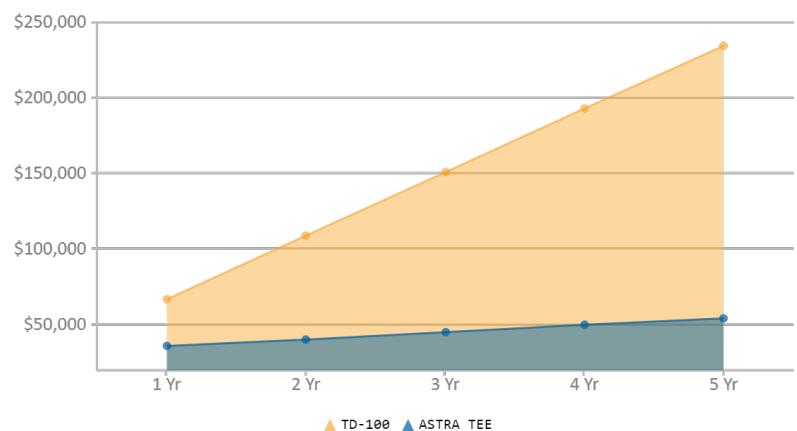

Compliant Workflow

Automated data logging and consumable tracking help you meet compliance standards. Clear, easy-to-follow steps guide the disinfection process



Optimized Speed

Disinfect up to 2 probes at a time for fast turnaround and increased efficiency. 10 to 13 minute* total reprocessing time without sleep cycles



Significant Savings

Helps reduce long-term operating costs with reusable, off-the-shelf disinfectant compatibility: RESET (hydrogen peroxide), CIDEX OPA and MetriCide OPA




CIVCO.com | info@civco.com | 1.800.445.6741

*total time depends on disinfection method used and water pressure



Detailed Comparison

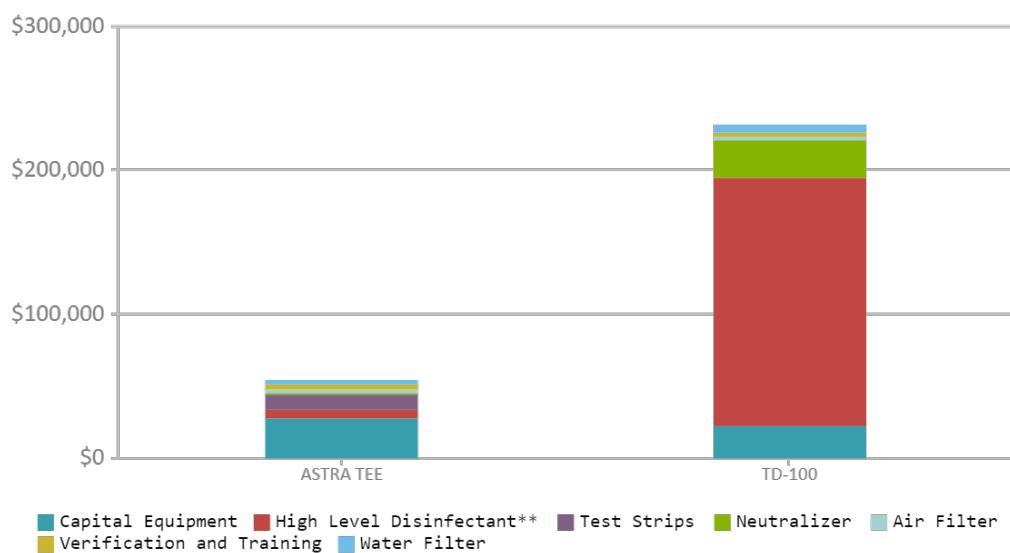

	ASTRA TEE	TD-100
Capital Equipment	\$27,800	\$22,479
High Level Disinfectant**	\$6,078	\$172,536
Test Strips	\$10,465	\$0
Neutralizer	\$1,170	\$26,026
Air Filter	\$2,445	\$2,614
Verification and Training	\$3,635	\$2,736
Water Filter	\$2,965	\$5,555

**High-level disinfectant used in TD-100 cost estimate is based on the TD-5 disinfectant. TD-5 is not owned or distributed by CIVCO Medical Solutions.



CIVCO.com | info@civco.com | 1.800.445.6741

COPYRIGHT © 2019. ALL RIGHTS RESERVED. CIVCO IS A REGISTERED TRADEMARK OF CIVCO MEDICAL SOLUTIONS. ASTRA IS A TRADEMARK OF CIVCO. TD100®, TD-5® AND TD-8® ARE OWNED BY CS MEDICAL, LLC AND ARE NOT DISTRIBUTED BY CIVCO. ALL OTHER TRADEMARKS ARE THE PROPERTY OF THEIR RESPECTIVE OWNERS. ALL PRODUCTS MAY NOT BE LICENSED IN ACCORDANCE WITH CANADIAN LAW. 2019R-3130 REV 1